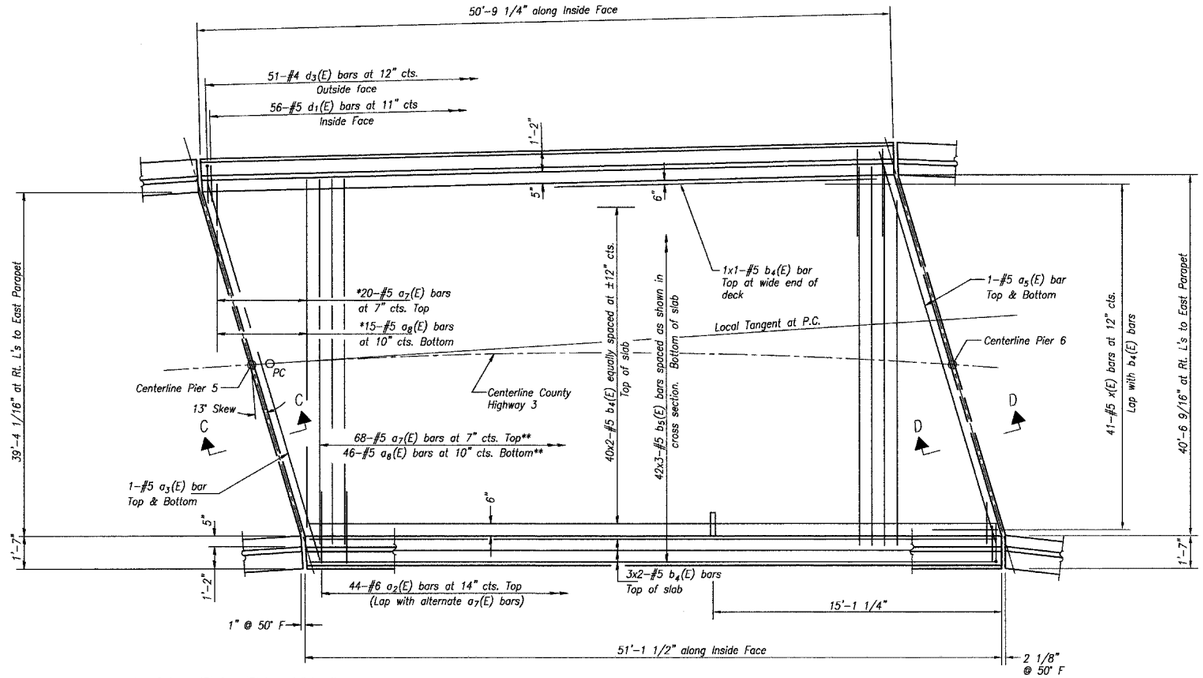

* Order a_7(E) & a_8(E) bars full length. Cut to fit skew and use remainder of bars in opposite end.

** Field cut a_7(E) & a_8(E) bars to fit bridge deck flare.

Min. Lap
#5 bars 1'-8"

PLAN

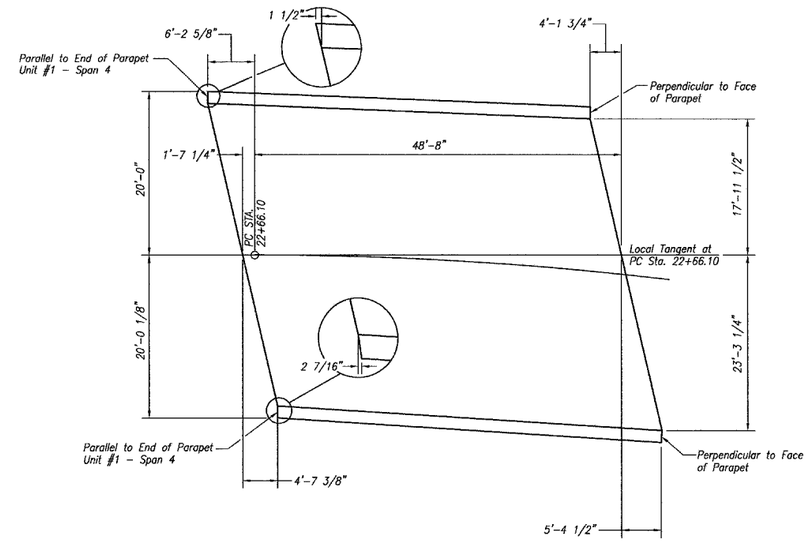

DECK LAYOUT DETAIL
UNIT #2 - SPAN 2

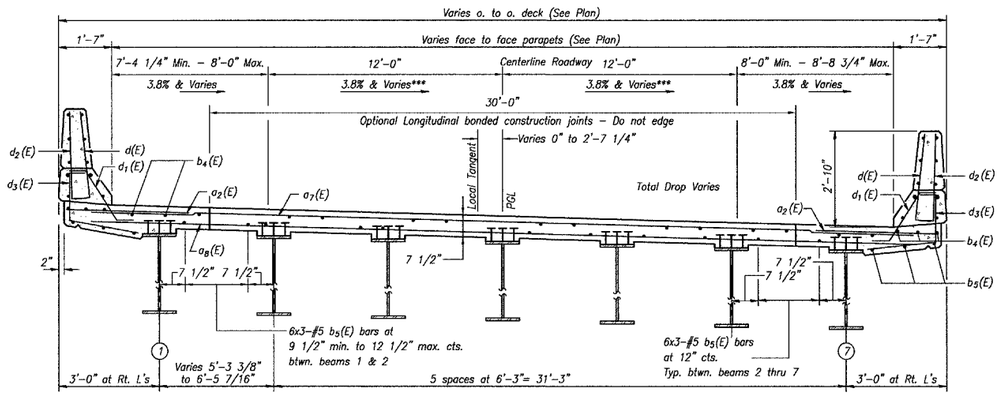

CROSS SECTION
(Looking North)

*** CROSS SLOPE VARIES DUE TO SUPERELEVATION TRANSITION. SEE SHEET 1 OF 38.

NOTE: Centerline Roadway and PGL will not always be on on centerline beam 4.

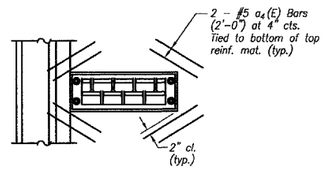

REINFORCEMENT DETAIL AT DRAINAGE SCUPPERS

Notes:

See Sheet #11 of 38 for Superstructure Details.

Reinforcement bars designated (E) shall be epoxy coated.

Bars indicated thus 20 x 3-#5 etc. indicates 20 lines of bars with 3 lengths per line.

See Sheet #12 of 38 for parapet reinforcement.

For Bent Bar Details and Bill of Materials See Sheet #13 of 38.

SUPERSTRUCTURE DETAILS
UNIT #2-SPAN 2
FAS 259 C.H. 3
OVER FOX RIVER
LA SALLE COUNTY
STA. 20+15.00
STRUCTURE NO. 050-3562

DRAWN BY: LAG	CAD: SUP3.DWG	REVISIONS DATE / BY		SCALE: AS NOTED	SHEET 34
		3/08/04	NET		
CHECKED BY: JKC	DATE: 02/03	7/06/04	NET	FILE NO.: 11174.01Y-1	OF 79